

Analysis of Total Mercury in Water by Cold Vapor Atomic Fluorescence Detection with the Brooks-Rand “MERX” Automated Mercury Analytical System

USGS-Mercury Research Laboratory
8505 Research Way
Middleton, Wisconsin 53562
mercury@usgs.gov
(608) 821-3844

Scope and Application

The following standard operating procedure (SOP) is used by the U.S. Geological Survey's Mercury Research Laboratory (MRL) to determine total mercury (HgT) concentrations in water. This SOP describes the preparation of the sample and subsequent analysis. Samples are collected into Teflon bottles and preserved to 1% v/v with MRL-supplied Hydrochloric Acid. Bromine Monochloride (BrCl) is added to the sample and heated to 50°C for five days to release matrix-bound mercury and oxidize all forms of mercury to the Hg²⁺ oxidation state. Immediately prior to analysis, the BrCl is neutralized by the addition of Hydroxylamine Hydrochloride (NH₂OH·HCl). Following neutralization, Stannous Chloride (SnCl₂) is added to the sample to reduce the mercury from Hg²⁺ to Hg⁰. The volatile Hg⁰ is purged from the sample and captured onto a gold sand trap, desorbed, and detected by cold vapor atomic fluorescence spectrometry (CVAFS). Sample analysis is conducted by the Brooks-Rand "MERX" automated mercury analytical system. Quality assurance and control protocols are employed throughout sample preparation and analysis, including: laboratory practices to prevent sample contamination, method blanks, analytical replication, and analytical matrix spikes.

Laboratory Safety

Analysts who use the MRL must have read, understood, and signed the Chemical Hygiene Plan for the MRL prior to potential exposure to any chemicals. The analyst must have a thorough understanding of the required safety protocols for the lab chemicals prior to their use of the lab. Adequate personal protection equipment such as safety glasses, gloves, and chemical resistant clothing must be worn when exposure to hazardous chemicals are possible. Caution should always be exercised; chemicals are present in the laboratory and often in use by other analysts. Hazardous chemicals should only be handled by adequately trained personnel under a high volume fume hood with extreme caution.

Multiple safety concerns are present in the conduct of this method; detailed information is included for each reagent specific to the method later in this SOP, and additional safety information can be found in the safety data sheets (SDS) located in the lab. Mercury is a toxic metal and caution should be exercised to limit exposure during daily operations. While samples and working standards are relatively low in concentration, concentrated stock solutions containing elevated HgT levels are occasionally encountered. Concentrated HgT stock solutions should only be handled by experienced lab personnel. Additionally, other hazardous chemicals used in this method include concentrated strong acids, SnCl₂, and BrCl (a strong oxidizer). Finally, during analysis the automated sample introduction system may begin moving without warning and presents a mechanical hazard.

Equipment

Trace level mercury analyses of samples at parts per billion concentrations are susceptible to contamination. Equipment that comes into contact with samples or reagents should be free of residual mercury and can consist of (but not be limited to) Teflon, glass, and polycarbonate containers. Brand new and previously used Teflon equipment should be washed in acid before use. The equipment is first rinsed with tap water, and then cleaned by immersing in 4 N HCl heated to 65°C for at least 12 hours (48 hours for new Teflon equipment). Immediately following removal from the bath, equipment is completely immersed in reagent-grade water and then additionally triple-rinsed in reagent-grade water. After rinsing, each container is air dried under a mercury-free class 100 laminar flow hood. Dry equipment is stored double bagged in zip-type bags.

Reagents and Standards

Reagents

All reagents and/or dry chemicals used to make reagents must be of the highest purity available from the vendor and shown to be low in mercury. Upon receipt at the laboratory, containers will be marked with the date of receipt and stored in the appropriate areas. When reagents are mixed for use in this method, the person who mixes them will record the chemical contents and concentration, and initial and date the reagent container. Reagents and manufacture instructions follow below.

Reagent water (Milli-Q water): Ultra-pure reagent grade water containing less than 0.1 ng/L Hg with a resistance greater than 18 M Ω -cm. The water is delivered through a 0.2 μ m filter, as obtained from a Millipore Academic water-purification system or equivalent.

Hydrochloric Acid (HCl): EM Science Omni Pure HCl (containing less than 5 ng/L Hg) or equivalent.

Bromine Monochloride (BrCl): Dissolve 27.0 g of reagent grade Potassium Bromide (KBr) in a new 2.5 L bottle of concentrated HCl. Place a Teflon coated stir bar into the bottle and stir for 1 hour or until dissolved. Slowly add 38.0 g reagent grade Potassium Bromate (KBrO₃) to the bottle while stirring. CAUTION: This needs to be done slowly and in a fume hood because large quantities of free halogens are produced. Addition of KBrO₃ to the solution should produce a color change from orange to red to yellow. Cap bottle loosely, stir for an additional hour, and remove stir bar. BrCl is stored in the original acid container in the acid cabinet. Replace the original acid label with a preprinted BrCl label and record your initials and the date made.

30% w/v Hydroxylamine hydrochloride (NH₂OH*HCl): Dissolve 120 g of NH₂OH*HCl in a Teflon bottle containing 400 mL of reagent grade water. Hydroxylamine hydrochloride typically contains significant amounts of HgT and needs to be treated to reduce the contamination to acceptable levels (< 0.02 ng/ml). Add 50 µL SnCl₂ to the solution and purge with Argon gas (300 mL/min for 1 hour). After the solution has been purged, analyze 0.1 ml in reagent water. If necessary, repeat the SnCl₂ addition and purging steps until the solution is below the acceptable level. Store the NH₂OH*HCl solution in the refrigerator when not in use.

20% w/v Stannous chloride (SnCl₂): Dissolve 200 g of SnCl₂ in 100 mL concentrated HCl in a 1 L Teflon bottle. Add 900 mL reagent water. Purge for 1 hour with Nitrogen gas at 300 mL/min. Store the SnCl₂ solution in the refrigerator when not in use.

Soda lime: Purchased from Alpha Aesar, 4-8 mesh.

Argon (Ar): Grade 5.0 (ultra high purity) Argon gas that is scrubbed of gaseous mercury by passing through a gold bead trap.

Nitrogen (N₂): Nitrogen gas is provided by a Peak Scientific nitrogen generator (model NM32LA) and is scrubbed of gaseous mercury by passing through a gold bead trap.

Analytical and Quality Control Standards

Upon receipt at the laboratory and on the day of preparation, mercury standard solutions should be labeled with the concentration, date received/prepared, and analyst initials. All standards must also be assigned a unique letter-number-letter identification code and must be entered into the laboratory database system. Concentrated (> 10 ng/ml) standard solutions should be stored outside of the main laboratory area to avoid contamination of the lab. Dispose of the working and concentrated mercury solutions in the appropriate waste container when expired (>6 months old for working solutions) or when the solution no longer contains BrCl (yellow color has faded to clear). Two standard solutions from different sources are required for analysis: an “analytical standard” which is used to calibrate the instrument and for matrix spikes, and a “quality control standard” which is purchased from a separate source and used to validate instrument performance throughout analyses.

Stock mercury standard solutions: The stock mercury standard solutions are commercially available mercury standards verified against a NIST standard reference material.

Working mercury standard solutions: The working mercury solutions are used in the daily operation of the instrument and are prepared from the stock solutions. The analytical standard and quality control standard (QCS) are prepared at 1 ng/ml (subsequent dilutions of the stock solutions may be necessary and should follow a

similar preparation). Dispense approximately 50 mL of reagent grade water and 3 mL of BrCl into a 100 mL mercury clean class A volumetric flask. Pipette the appropriate volume of stock solution (or diluted stock solution) and bring to volume with reagent water. Store the standard in a designated Teflon mercury standard bottle, and label with concentration, bottle identification code, date prepared, and analyst initials. Enter the working standard solutions into the lab database. This working standard must be compared to the previous working standard and agree within $\pm 5\%$. Prepare fresh every 6 months.

Sample Preparation

Analysis of waters for HgT requires the addition of BrCl to the sample (1.2% BrCl v/v) to oxidize all mercury to Hg²⁺. Samples with high visible levels of dissolved organic carbon are placed in an ultraviolet light box until colorless (this step may be skipped if the samples are colorless or nearly so). Prior to bromination, the HgT concentration of the BrCl should be determined by CVAFS analysis. The BrCl concentration, sample identification codes, and volume of BrCl added to each sample should be logged into the lab's database. Following bromination, samples are placed into a convection oven and heated to 50°C for five days. If the yellow color remains after five days, this indicates excess BrCl in the sample and it is ready for analysis. If the yellow color is absent, additional BrCl is added and the sample is again placed in the oven overnight. Additions of BrCl must be repeated until the sample color indicates the presence of excess BrCl.

Instrument Operation

The MERX instrument consists of three interconnected modules: the autosampler, trap/desorption unit, and the detector. The instrument is designed to operate on a specific mixture of reagents that are prepared in septa sealed 42 ml glass vials. The autosampler holds three removable 24 vial sample racks, each consisting of 3 rows of 8 vials. Vial number one is the upper right position, with vial position descending from right to left, then top to bottom. Once prepared, the vials are sealed to the atmosphere and remain viable for analysis up to 48 hours. A typical analytical run is shown in Appendix 1.

Start Up

1. Check that all modules of the instrument have power and the Argon gas supply is turned on.
2. Open the Mercury Guru4 software with the shortcut on the desktop.
3. Open the analytical template file "water.brt" for water analysis in the File drop down menu (File→Open→Merx→Template)

4. Save the file as data (File→"save file as data" →Merx→Runs→2016) in the data folder from the current year. Name the new run file by date and sample description (MMDDYY_sample name.brd).
5. From the "Instrument" dropdown menu, select "Connect", prompting a popup window displaying three communication ports. Select the appropriate ports (CVAFS = COM4, Purge and Trap = COM5, and Autosampler = COM6) and click "Accept". The communication status at the top of the screen will turn green indicating connection with each module.
6. In the automation page of the Guru software, click the Argon gas button to start gas flow to the detector. Adjust the sensitivity of the detector so the baseline offset is approximately 3000 by changing the PMT value (use the up/down arrows on the front of the detector). When the PMT value is changed, the offset value will go blank, and the new offset value will temporarily appear in the signal field. Press the autozero button when the signal value is 3000. Allow the signal to stabilize (2-3 minutes), and then measure the instrument noise (found in the "File" dropdown menu). Record the new offset, PMT, and noise values in the instrument log notebook.
7. Replace the Soda Lime in the trap on the front of the instrument.

Initial Instrument Calibration

1. Put 20 new 42 ml glass vials into a sample rack. Remove the caps and put into a clean bag.
2. Add 100 μl of $\text{NH}_2\text{OH}\cdot\text{HCl}$ and 20 ml of reagent water to vials 5-20 (leave the first four vials empty).
3. Create a six point calibration curve in vials 9-14 using the analytical working standard (generally a 10-400 pg calibration curve is sufficient for most samples).
4. Add QCS checks in vials 19-20 that are near the low and high ends of the calibration curve.
5. Add 100 μl of SnCl_2 to vials 5-20, and seal all vials promptly.
6. Vials 7,8, 17, and 18 are used as blanks for instrument calibration. Vials 1-6 and 15-16 are instrument blanks and are not used for instrument calibration.
7. Install the sample rack in the autosampler, making sure that it is orientated properly.

8. Update the "Name/ID" field in the sample information page in the Guru software.
9. In the automation page, select the start vial number (1) and the number of vials to be analyzed (20), and click start analysis.
10. Enter the results into the appropriate Excel spread sheet (see "Data Management" section below). Review the calibration curve and QCS check standards in the Excel sheet; proceed with sample analysis only if all quality control parameters are met.

Sample Analysis

1. Select 10 samples for analysis (see Appendix 1 to determine analysis order). Be careful not to use a field blank in the duplicate/spike position.
2. Put 16 new 42 ml glass vials into a sample rack. Remove the caps and put into a clean bag.
3. Add 100 μl of $\text{NH}_2\text{OH}\cdot\text{HCl}$ to each vial.
4. Using a balance, weigh 15-20 ml of sample into each of the appropriate vials. When adding less than 10 ml of sample, it is necessary to use a pipette to maintain three significant figures in the data output. If less than 15 ml of sample is added, add reagent water to bring the volume up to 20 ml. Do not exceed 25 ml of volume in the analytical vials as that may flood the instrument. Record the mass of sample added to each vial in the analytical volume field of the Excel spread sheet (see next section for further details).
5. Pipette 20 ml of reagent water into the bubbler blanks (vials 7 and 14) and the QCS check vials (vials 15-16).
6. Add the QCS check standards and the instrument spike to the appropriate vials.
7. Add 100 μl of SnCl_2 to each of the vials and promptly cap.
8. Install the sample rack in the autosampler, making sure that it is orientated properly.
9. In the automation page, select the start vial number and the number of vials to be analyzed, and click start analysis.

Data Management

1. Data created on the Merx should be recorded in an Excel analytical spread sheet. Open the template for water analysis (Merx→XL runs→2016→"MERX water template.xls"). Save the Excel file in the same folder with a new name that includes the date and sample description (MMDDYY_sample name.xls).
2. In the Excel spread sheet, fill out the header information and the amount of mercury used to create the calibration curve (as mass, in nanograms).
3. In the Excel spread sheet, enter the sample barcodes and volumes of samples/QCS analyzed.
4. The analysis spread sheet has designated rows for duplicates, instrument spikes, equipment blanks, and QCS checks standards. These fall in the appropriate places in the run and should not be used for sample analyses.
5. As the analysis progresses, data will appear in the "results" page of the Guru software. To avoid typographical error, data should be copied from a report created by the Guru software. Create the report from the "reports" page of the Guru software (click "create a report", select the .csv output, and navigate to Merx→XL runs→2016). Save the report and name by date and sample description (MMDDYY_sample name.csv).
6. Copy the peak areas from the report file generated by the Guru software and paste into the Peak Area column of the spread sheet. See Appendix 3 for an example of a completed Excel file.

Quality Assurance and Control Protocols

Analytical Precision: One sample should be analyzed in duplicate for every 10 samples analyzed. The percent difference for duplicate samples should be less than 10%. In the case of failure, repeat the duplicate and bring to the attention of the quality assurance officer.

Matrix Interference: One sample should be analyzed as an instrument spike for every 10 samples analyzed to assess for matrix interference. The sample that was analyzed in duplicate should be set up a third time and spiked with 100 pg of the analytical mercury standard. The recovery of the spike should be within 85 – 115 % of the known addition. In the case of failure, repeat the duplicate spike in the failed sample and in another sample from the set and bring to the attention of the quality assurance officer.

Instrumental Carryover: Instrumental carryover is assessed with instrument blank samples analyzed throughout the run. A blank sample is the analysis of reagent water (with $\text{NH}_2\text{OH}\cdot\text{HCl}$ and SnCl_2). Excessive instrumental carryover (peak areas two times greater than the instrument calibration blanks) indicates instrumental contamination with HgT.

Instrument Calibration: Calibrate the instrument with a 6 point standard curve prior to sample analysis and conduct regular checks of instrument calibration throughout the run (QCS check standards). A standard curve should be created with masses of HgT that span that of the samples, and have an r^2 value greater than 0.995. Two QCS check standards should be analyzed following every 10 samples to verify instrument calibration, and have concentrations of 90 – 110% of its true value. The failure of subsequent check standards is an indication of instrumental drift which may require recalibration of the instrument. If a sample exceeds the instrument calibration, either the sample should be repeated at lower volume or the instrument recalibrated with higher masses of HgT.

APPENDIX 1. Example of a typical analytical run.

Instrument Calibration

| | | | | | | | |
|---------------------------------|---------------------------------|-------------------------------------|-------------------------------------|-------------------------------------|-------------------------------------|-------------------------------------|------------------------------------|
| <u>8</u> Calibration blank 2 | <u>7</u> Calibration blank 1 | <u>6</u> Instrument blank | <u>5</u> Instrument blank | <u>4</u> Empty vial | <u>3</u> Empty vial | <u>2</u> Empty vial | <u>1</u> Empty vial |
| <u>16</u> Instrument blank | <u>15</u> Instrument blank | <u>14</u> Calibration standard 6 | <u>13</u> Calibration standard 5 | <u>12</u> Calibration standard 4 | <u>11</u> Calibration standard 3 | <u>10</u> Calibration standard 2 | <u>9</u> Calibration standard 1 |
| <u>24</u> | <u>23</u> | <u>22</u> | <u>21</u> | <u>20</u> QCS standard | <u>19</u> QCS standard | <u>18</u> Calibration blank 4 | <u>17</u> Calibration blank 3 |


Sample Rack 1

| | | | | | | | |
|-------------------------------------|-------------------------------|----------------------------------|------------------------|------------------------|------------------------|------------------------|------------------------|
| <u>32</u> Sample 5 matrix spike | <u>31</u> Instrument blank | <u>30</u> Sample 5 duplicate | <u>29</u> Sample 5 | <u>28</u> Sample 4 | <u>27</u> Sample 3 | <u>26</u> Sample 2 | <u>25</u> Sample 1 |
| <u>40</u> QCS standard | <u>39</u> QCS standard | <u>38</u> Instrument blank | <u>37</u> Sample 10 | <u>36</u> Sample 9 | <u>35</u> Sample 8 | <u>34</u> Sample 7 | <u>33</u> Sample 6 |
| <u>48</u> Sample 15 matrix spike | <u>47</u> Instrument blank | <u>46</u> Sample 15 duplicate | <u>45</u> Sample 15 | <u>44</u> Sample 14 | <u>43</u> Sample 13 | <u>42</u> Sample 12 | <u>41</u> Sample 11 |

Sample Rack 2

| | | | | | | | |
|---------------------------|---------------------------|-------------------------------|------------------------|------------------------|------------------------|------------------------|------------------------|
| <u>56</u> QCS standard | <u>55</u> QCS standard | <u>54</u> Instrument blank | <u>53</u> Sample 20 | <u>52</u> Sample 19 | <u>51</u> Sample 18 | <u>50</u> Sample 17 | <u>49</u> Sample 16 |
| <u>64</u> | <u>63</u> | <u>62</u> | <u>61</u> | <u>60</u> | <u>59</u> | <u>58</u> | <u>57</u> |
| <u>72</u> | <u>70</u> | <u>70</u> | <u>69</u> | <u>68</u> | <u>67</u> | <u>66</u> | <u>65</u> |

APPENDIX 2. Example of a completed Excel data sheet for water analysis.

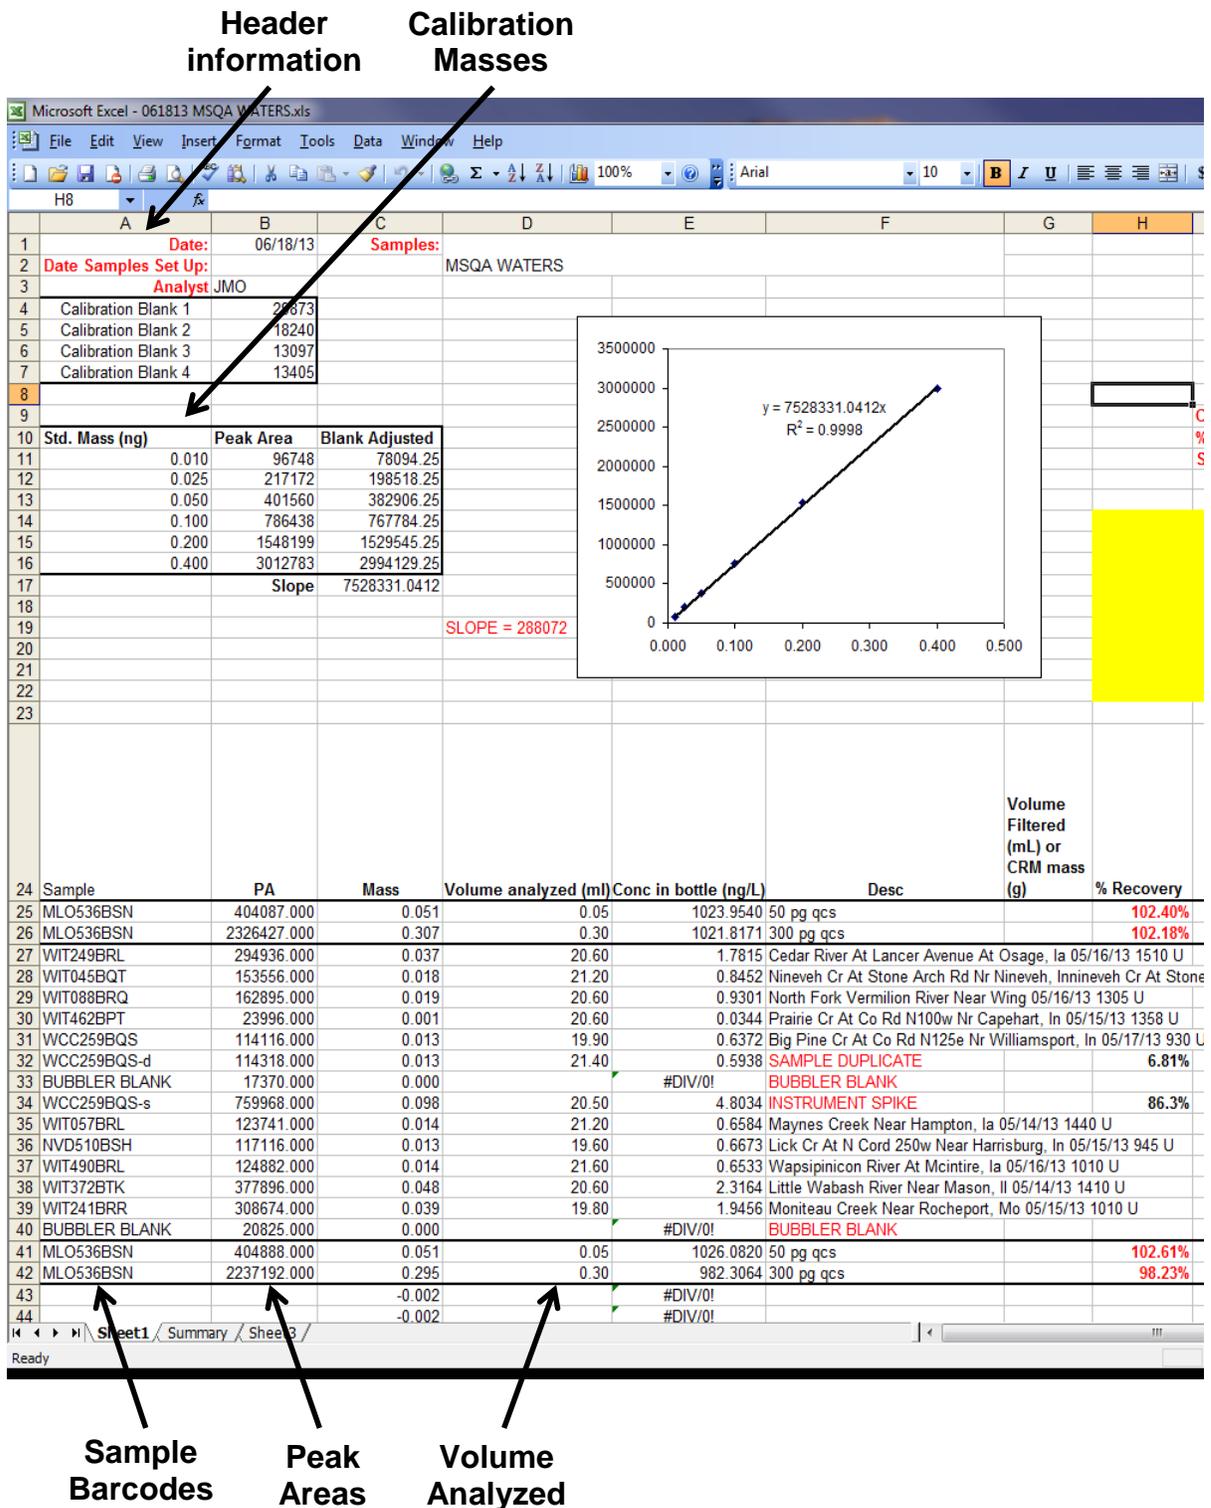

Appendix 4. Definition of equations.

$$\text{Sample Hg Concentration} = \frac{(\text{Analytical Hg Mass})}{(\text{Volume Analyzed})}$$

$$\text{Analytical Hg mass} = \frac{(\text{Sample Peak Area}) - (\text{Mean Calibration Blanks Peak Area})}{(\text{Slope of Calibration})}$$

$$\text{Hg Spike Percent Recovery} = \frac{\left(\frac{\text{Analytical Hg Mass of Spiked Sample Aliquot}}{\text{Sample Aliquot}} \right) - \left(\frac{\text{Hg Concentration of Unspiked Sample Aliquot}}{\text{Sample Aliquot}} \right) (\text{Volume of Spiked Sample Aliquot})}{(\text{Spike Mass})} \times 100$$

$$\text{Duplicate Percent Difference} = \frac{(\text{Hg Concentration of Sample}) - (\text{Hg Concentration of Duplicate})}{(\text{Hg Concentration of Sample})} \times 100$$

$$\text{Percent Recovery} = \frac{(\text{Analyzed Concentration})}{(\text{Known Concentration})} \times 100$$